



FIG. 8A




FIG. 8B

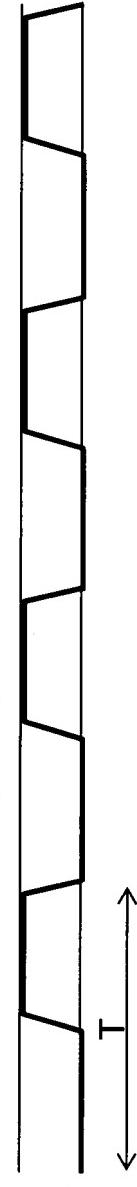


FIG. 8C




FIG. 8D




FIG. 8E



(a) Pulse voltage for scan electrodes (when supplied from aging device)

FIG. 10A




(b) Pulse voltage for sustain electrodes (when supplied from aging device)

FIG. 10B



(c) Pulse voltage for scan electrodes (immediately before

FIG. 10C

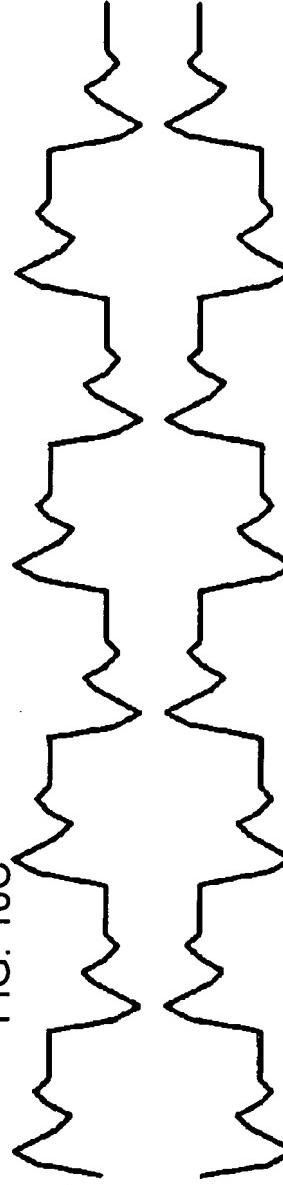

(d) Pulse voltage for sustain electrodes (immediately before

FIG. 10D

